

**More control,
less stress.**



Evolution® Duodenal

CONTROLLED-RELEASE STENT - UNCOVERED



www.cookmedical.com

More control, less stress.

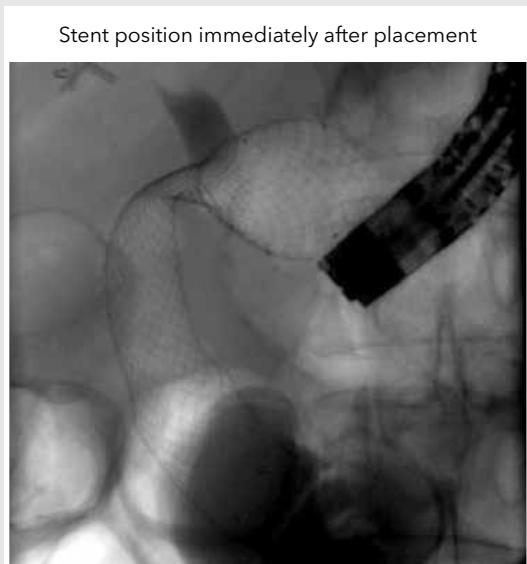


Image courtesy of Prof. Horst Neuhaus,
Evangelisches Krankenhaus Medizinische Klinik,
Düsseldorf


The braided-to-coiled construction of the Flexor allows for unparalleled trackability and maneuverability for deployment in difficult angulations

Rounded tip design to reduce trauma and to aid in traversing abnormal anatomy

4 radiopaque markers at each end provide visualization for more precise placement

Evolutionary Design

Evolution is designed with 18 crowns (atraumatic looped ends) for enhanced, evenly distributed radial force and better wall apposition. This allows the stent to adapt to the natural curves of the anatomy while potentially reducing the risk of delayed perforation.

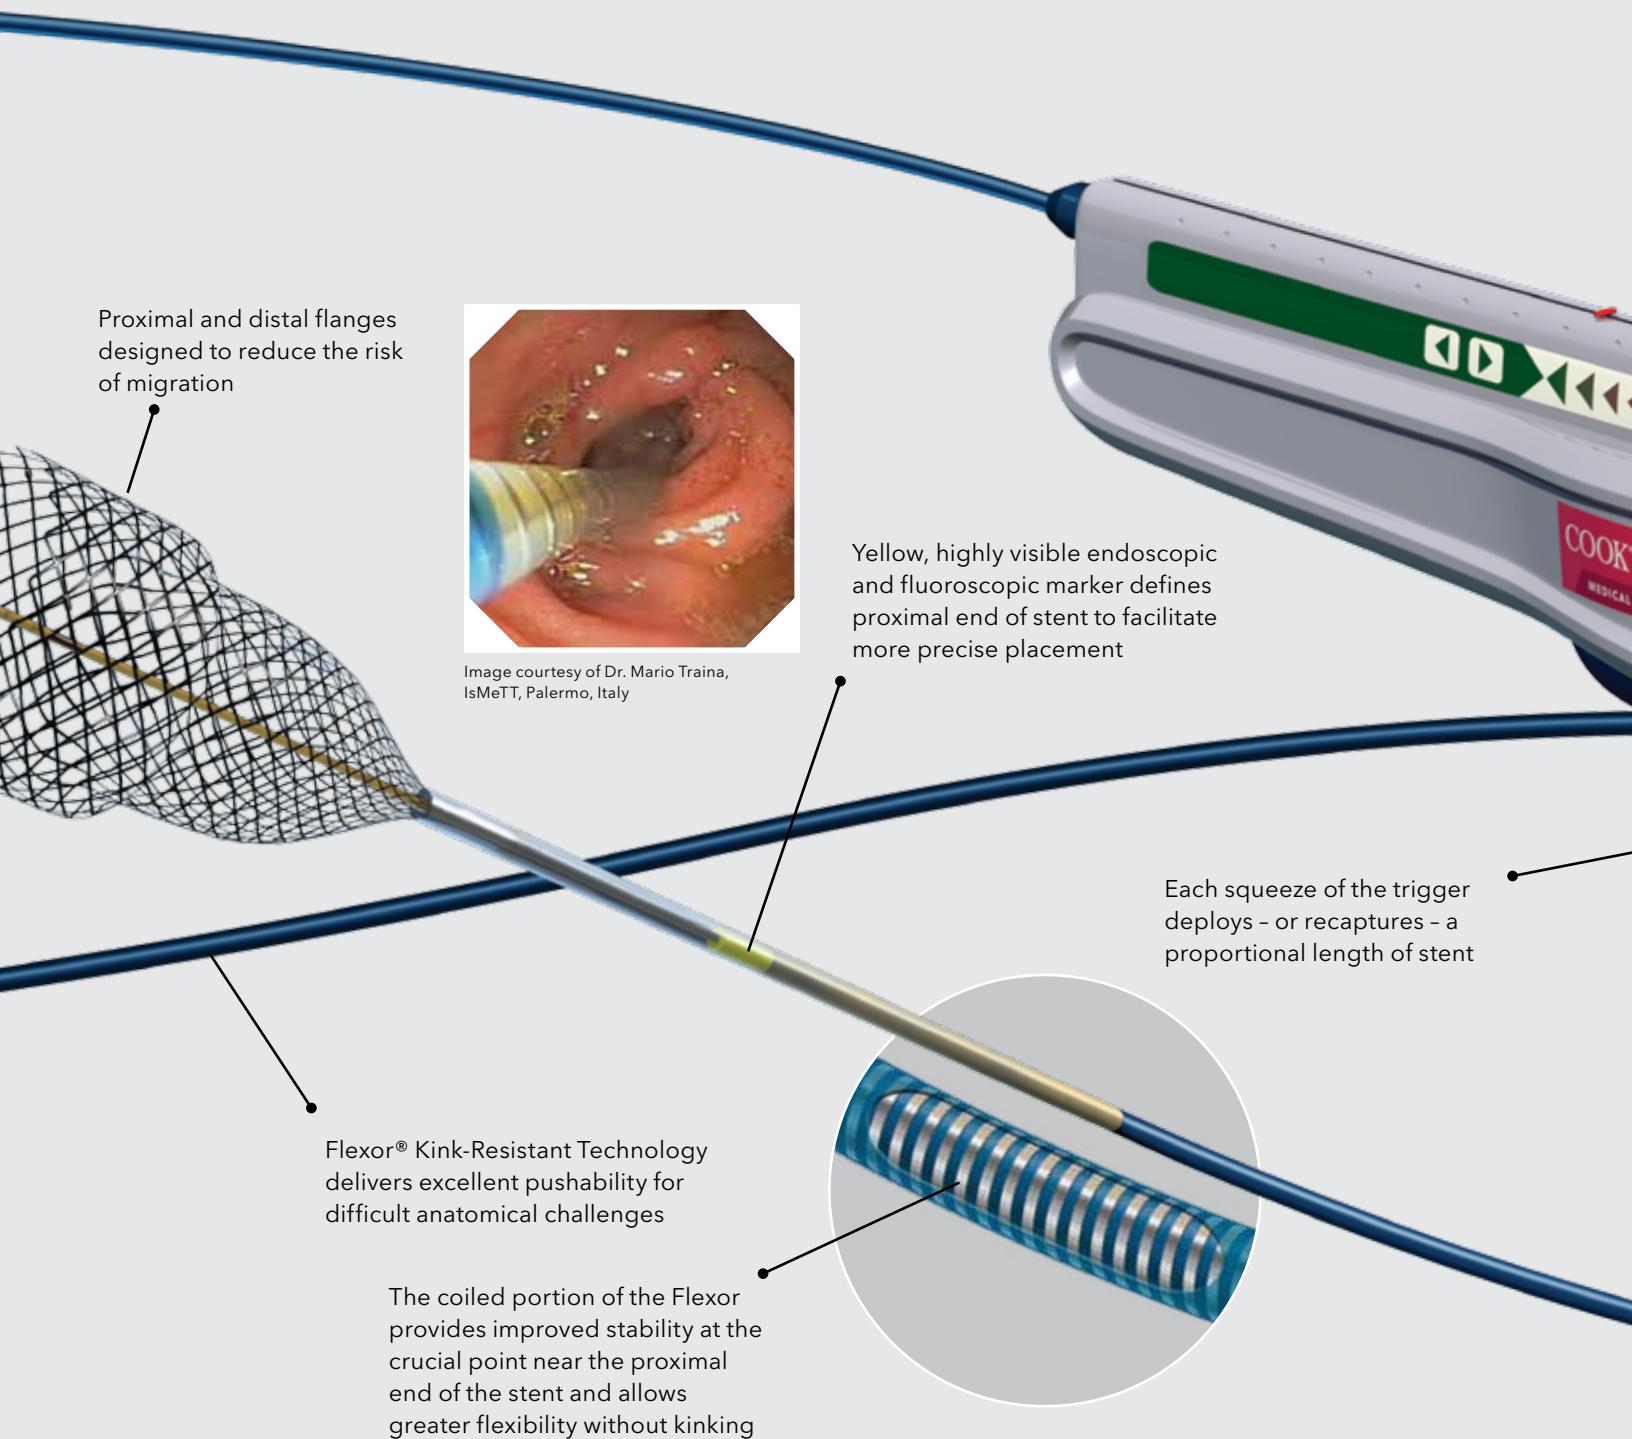

Evolutionary Control

With Evolution - the only stent delivery system with our controlled release and recapturability - you will experience unprecedented precision and trackability during stent placement. Every action applied to the trigger-based handle causes a precise reaction to ensure the stent will be placed correctly.

"Point-of-no-return" mark
alerts you when recapture
is no longer possible


Safety wire secures the stent
to the handle, ensuring stent
recapturability

Directional button allows you to
easily shift from deployment to
recapture mode and back again



Evolutionary Security

Whether you're confronting malignant strictures or gastric outlet obstruction caused by malignancy, the Evolution Controlled-Release Stent delivers the control and maneuverability you need to confidently deliver a stent that provides better wall apposition and fully conforms to the natural curves of the anatomy while potentially reducing post-placement risks.

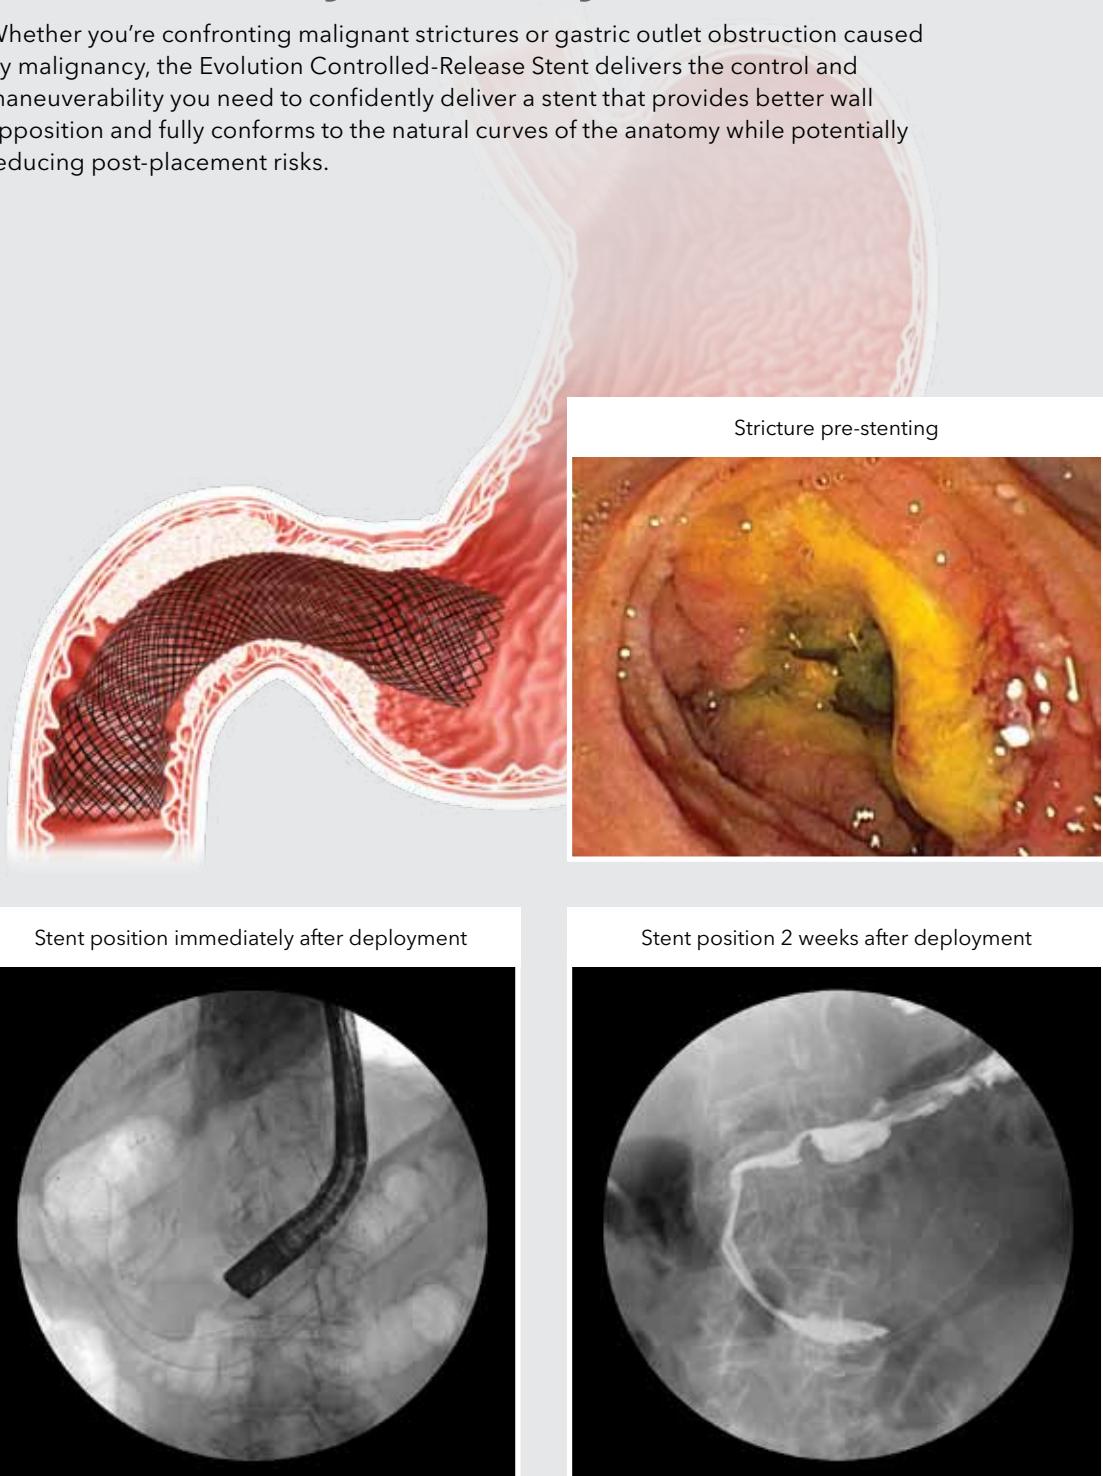

Product Specifications

Used for palliative treatment of duodenal or gastric outlet obstruction and duodenal strictures caused by malignant neoplasms.

Supplied sterile and is disposable - intended for single use only.

Order Number	Reference Part Number	Body Diameter mm	Flange Diameter mm	Stent Length cm	Delivery System Fr	Delivery System Length cm
G48025	EVO-22-27-6-D	22	27	6	10	230
G48026	EVO-22-27-9-D	22	27	9	10	230
G48027	EVO-22-27-12-D	22	27	12	10	230

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

Customer Service

EMEA: EDI - www.cookmedical.com/edi.do
Distributors: +353 61239240, ssc.distributors@cookmedical.com
Austria: +43 179567121, oe.orders@cookmedical.com
Belgium: +32 27001633, be.orders@cookmedical.com
Denmark: +45 38487607, da.orders@cookmedical.com
Finland: +358 972519996, fi.orders@cookmedical.com
France: +33 171230269, fr.orders@cookmedical.com
Germany: +49 6950072804, de.orders@cookmedical.com
Hungary: +36 17779199, hu.orders@cookmedical.com
Ireland: +353 61239252, ie.orders@cookmedical.com
Italy: +39 0269682853, it.orders@cookmedical.com
Netherlands: +31 202013367, nl.orders@cookmedical.com
Norway: +47 23162968, no.orders@cookmedical.com
Spain: +34 912702691, es.orders@cookmedical.com
Sweden: +46 858769468, se.orders@cookmedical.com
Switzerland - French: +41 448009609, fr.orders@cookmedical.com
Switzerland - Italian: +41 448009609, it.orders@cookmedical.com
Switzerland - German: +41 448009609, de.orders@cookmedical.com
United Kingdom: +44 2073654183, uk.orders@cookmedical.com

www.cookmedical.com

Americas: EDI - www.cookmedical.com/edi.do
Phone: +1 812.339.2235, 800.457.4500, Fax: 800.554.8335
E-mail: orders@cookmedical.com

Australia:
Phone: +61 738411188, 1800077222, Fax: +61 738411288, 1800077283
E-mail: cau.custserv@cookmedical.com

